

Dedicated to Delivery
Nasco
Life/form®

3 *Life/form.*
Year
Warranty
Simulators
& Trainers

Pediatric Injection Training Arm Simulator — LF00958U Instruction Manual





DO NOT REMOVE FILM FROM TUBING!
THIS PRODUCT CONTAINS DRY NATURAL RUBBER!

Life/form® Products by **Nasco**

About the Simulator

The **Life/form**® Pediatric Injectable Training Arm Simulator is a dramatic and exciting training aid for practicing and demonstrating intramuscular and intravenous puncture of young children. Visual as well as tactile realism have been designed into this training aid to provide students with the most realistic training possible in developing skills for pediatric IM and venipuncture. A special, extremely thin synthetic skin is paired with rubber tubing with small lumen and thin walls to make the **Life/form**® Pediatric Injectable Training Arm Simulator the most realistic means of training medical personnel available.

With proper care, this **Life/form**® Simulator will provide years of reliable service. Please read the instructions carefully.

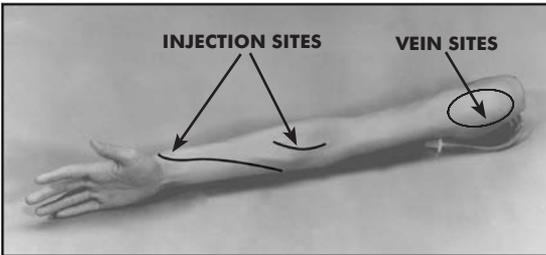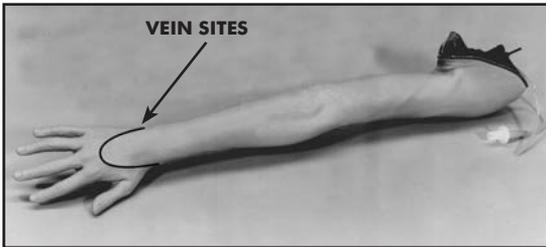

List of Components

- **Life/form**® Arm with White Skin
- Blood Donor Set
- 3 cc Syringe
- **Life/form**® Venous Blood — 1 Pint
- IV Bag


Internal Structure

The photos on the lower left show the position of tubing embedded within the arm to simulate veins. The tubing is superficial in its full length, offering a wide selection of injection sites. Careful palpation should allow the student to locate the veins.


General Instructions for Use




- A. Prepare Synthetic Blood**
Concentrated blood colorant is provided. Fill the 16-oz. container with water for proper dilution.

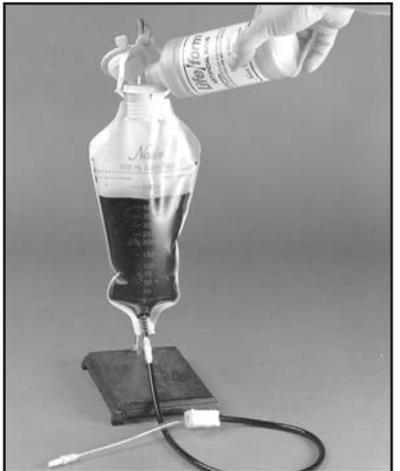

- B. Fill and Prepare IV Supply Bag**
Pour diluted **Life/form**® blood into IV container.

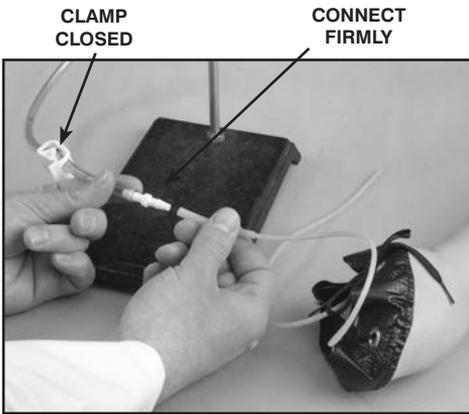

Procedures That Can Be Performed on This Simulator

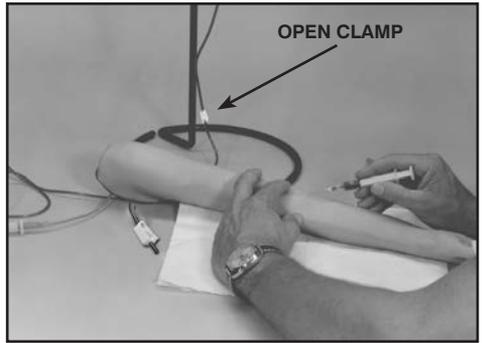


C. IV Bag

Hang bag at 18" height. Be certain clamp on administration set is closed before hanging.

D. Connect to Arm

The arm is supplied with a special connector that fits arm tubing and IV tubing. Insert connector from IV tubing into tubing coming from arm as shown.

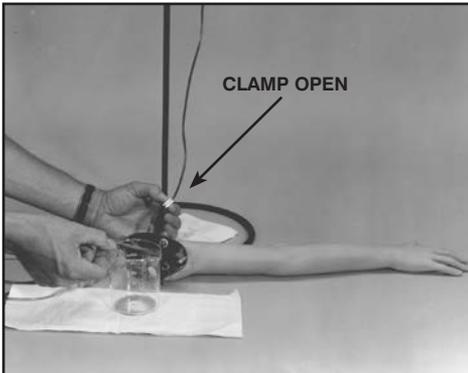


E. Fill Venous System

1. Hold open end of shoulder tubing over container.
2. Open clamp and allow **Life/form**® Blood to flow through system until steady stream exits without bubbles through the open tubing end.
3. Place pinch clamp on open tubing end.

A. Venipuncture

The **Life/form**® Pediatric Injectable Training Arm Simulator is now pressurized and ready for venipuncture practice. Venous pressure is altered by varying the height of the IV bag. A height of 18" is a good starting point. Excessive height may cause leakage through previous puncture sites. Needle sizes should be kept as small as possible to minimize damage to the arm skin and tubing. Refer to pg. 1 for identification of vein sites.

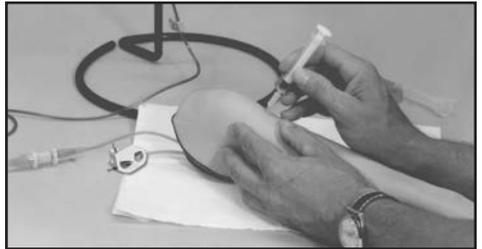

B. Intramuscular Injections

The **Life/form**® Pediatric Injectable Training Arm Simulator has been designed to include a soft foam area in the shoulder to simulate the deltoid muscle and allow practice for intramuscular injections. The injection area can be easily located by palpation. Although fluids may be used for IM injections in this arm, it is recommended that air be used when possible to prevent build-up of fluids in the arm. If fluid is to be used, distilled water is recommended, and the arm should be allowed to drain before storing.

Causes for Failure in Function

- A.** IV infusion may not flow if there is air in the venous system. Simply flush the system slowly with more synthetic blood or distilled water, whichever you are using. Be sure to check the IV bag clamp; it might have been overlooked and not opened.
- B.** During procedure of drawing blood, if blood cannot be aspirated:
1. The clamp on the IV tubing of the synthetic blood might not be opened.
 2. Air could be trapped in the venous system. Simply flush the system slowly, draining some blood or distilled water, whichever you are using, until all air bubbles are eliminated.
 3. If blood flow is weak, the pressure can be increased by raising the supply bag to a higher level. Only raise the bag enough to achieve desired flow.
 4. If these measures do not unclog the venous system, try using a large (50 cc) syringe to force fluid through the tubing.
 5. If none of these measures work, peel off the skin to the knuckles. **DO NOT REMOVE FROM FINGERS.** Examine all tubing for possible kinks that occasionally occur during assembly. Soap up outside of arm core generously with Ivory® liquid detergent and pull skin over arm core.

Care of Simulator

This training simulator has been designed to provide the greatest possible durability and lowest maintenance while not compromising the realism of use. Following are some suggestions for helping you yield the maximum life from this unique simulator.



A. Before Storing Arm

1. Disconnect IV bag and pour fluid back into container.
2. Rinse IV bag.
3. Drain arm. Open pinch clamp and tip hand up until fluid is removed. Flush arm with water. Rinse off exterior of arm, dry, and return arm to storage bag.
4. Return all components to case.

B. Needles

Hypodermic needles are actually small cutting tools. Puncturing the skin and vein with needles results in small cuts or slits which will eventually lead to deterioration. The larger the needles, the larger the cuts made in the skin and the shorter the life of the simulator. It is recommended that 24-gauge or smaller needles be used. Always use sharp needles. Dull or bent needles cause excessive tearing.

C. Distribution of Punctures

The vein is in contact with the skin from the point it enters the arm to the point of exit. If the injections are distributed along the length of the vein, without deviation from acceptable practice, the product will last longer.

D. Tubing Sealant

Tubing Sealing (LF01099U) has been developed for use with **Life/form®** Injectable Simulators. It will effectively seal punctures in tubing.

E. Skin Replacement

After prolonged use for injections, the skin on your training arm will show track marks and need replacing with Replacement Skin and Vein Kit (LF00986U).




1. Remove used skin from arm.
 - a. Untie lace at shoulder.
 - b. Lubricate exterior of skin with Ivory® liquid detergent.
 - c. Peel skin off by turning inside out.
 - d. Remove old tubing.



2. Install new tubing.

Place new section of tubing in channel of arm core. Be certain equal portions of tubing protrude at shoulder.

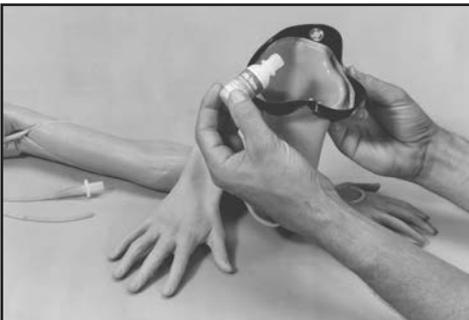


3. Lubricate skin.

Pour contents of the bottle of **Life/form**® Simulator Lubricant provided inside arm skin and swish around to coat all inside surfaces.




4. Install new skin.
 - a. Slide shoulder of skin over head of core. Be certain to align palm of core and skin.
 - b. Grasp the skin with both hands and slide over core until fingers of core approach finger holes of skin.

CAUTION: The thin **Life/form**® Skin used to provide realism is tender and care must be taken not to stretch or tear the material when installing.

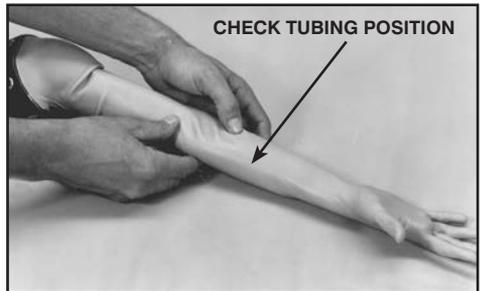

- c. Check tubing location. If tubing has moved from channel, try to work into place by palpating through skin. If unsuccessful, peel skin back (invert) until tubing can be replaced properly, then roll skin over core.
- d. Work fingers into place.
- e. Draw skin snugly into place.

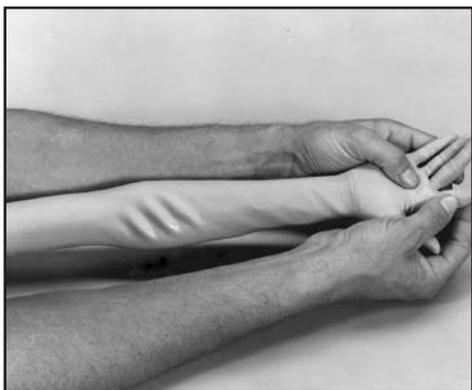

5. Install lace.

Thread lace through eyelets in alternating pattern, as illustrated, and tie snugly. Be certain tubing is protruding and not pinched by blowing through tubing.

6. Rinse.

Wash excess lubricant from exterior of arm skin. The **Life/form**® Pediatric Injectable Training Arm Simulator is now fully reconditioned and ready to train hundreds of new medical personnel.

**Supplies/Replacement Parts for
Life/form® Pediatric Injectable
Training Arm Simulator**

LF00986U	Replacement Skin and Vein Kit
LF01099U	Tubing Sealant
LF00845U	Life/form ® Venous Blood — 1 Quart
LF00846U	Life/form ® Venous Blood — 1 Gallon
LF09919U	Nasco Cleaner

Other Available *Life/form*® Simulators

- LF00698U** Adult Injectable Arm (White)
LF00855U Male Catheterization
LF00856U Female Catheterization
LF00901U Prostate Examination
LF00906U Ostomy Care
LF00929U Surgical Bandaging
LF00957U Enema Administration
LF00958U Pediatric Injectable Arm
LF00961U Intramuscular Injection
LF00984U Breast Examination
LF00995U Arterial Puncture Arm
LF00999U Pediatric Injectable Head
LF01005U First Aid Arm
LF01008U Intradermal Injection Arm
LF01012U Heart Catheterization (TPN)
LF01019U Ear Examination
LF01027U Peritoneal Dialysis
LF01028U Suture Practice Arm
LF01034U Suture Practice Leg
LF01036U Spinal Injection
LF01037U Hemodialysis Practice Arm
LF01038U Episiotomy Suturing Set
LF01042U Suture Kit
LF01062U Pelvic, Normal & Abnormal
LF01063U Stump Bandaging, Upper
LF01064U Stump Bandaging, Lower
LF01069U Cervical Effacement
LF01070U Birthing Station
LF01082U Cricothyrotomy
LF01083U Tracheostomy Care
LF01084U Sigmoidoscopic Examination
LF01087U Central Venous Cannulation
LF01095U Blood Pressure Arm
LF01108U Infant Intraosseous Infusion
LF01121U Advanced IV Arm
LF01131U Venipuncture and Injection Arm
LF01139U Advanced IV Hand
LF01142U Auscultation Trainer
LF01143U Testicular Exam
LF01152U Male & Female Catheter
LF01155U Advanced CPR Dog
LF01162U Venatech IV Trainer
LF01174U NG Tube & Trach Skills
LF01184U Venatech IM & Sub Q
LF01193U Special Needs Baby
LF03000U **CPARLENE**® Series
LF03601U Adult Airway Management Trainer with Stand
LF03602U Adult Airway Management Manikin
LF03609U Child Airway Management Trainer with Stand
LF03616U Child **CRISIS**™ Manikin
LF03617U Deluxe Child **CRISIS**™ Manikin with Arrhythmia Tutor
LF03620U PALS Update Kit
LF03623U Infant Airway Management Trainer with Stand
LF03632U Child Intraosseous Infusion/Femoral Access Leg on a Stand
LF03633U Child Airway Management Trainer Torso
LF03693U **Basic Buddy**® CPR Manikin
LF03699U "Airway Larry" Airway Management Trainer
LF03709U Infant **CRISIS**™ Manikin
LF03720U **Baby Buddy**™ Infant CPR Manikin
LF03750U Fat Old Fred
LF03760U Airway Management/Cricoid Pressure Trainer
LF03770U Chest Tube
LF03953U **CRISIS**™ Manikin, Complete
LF03955U Deluxe **CRISIS**™ Manikin
LF03956U Deluxe "Plus" **CRISIS**™ Manikin
LF03965U Adult **CRISIS**™ Auscultation Manikin
LF03966U Adult **CRISIS**™ Auscultation Manikin with ECG Simulator
LF04000U **GERI**™/**KERI**™ Manikin Series
LF04200U Adult Sternal Intraosseous Infusion
LF06001U CPR Prompt® Adult/Child Manikin
LF06012U CPR Prompt® Infant Manikin
LF06200U CPR Prompt® Keychain Rescue Aid
LF06204U CPR Prompt® Rescue and Practice Aid

Nasco Fort Atkinson

901 Janesville Avenue, P.O. Box 901
Fort Atkinson, Wisconsin 53538-0901
1-800-558-9595

eNasco.com • E-mail: lifeform@eNasco.com